




E.coli O157 Plus Procedure

TEST PROCEDURE

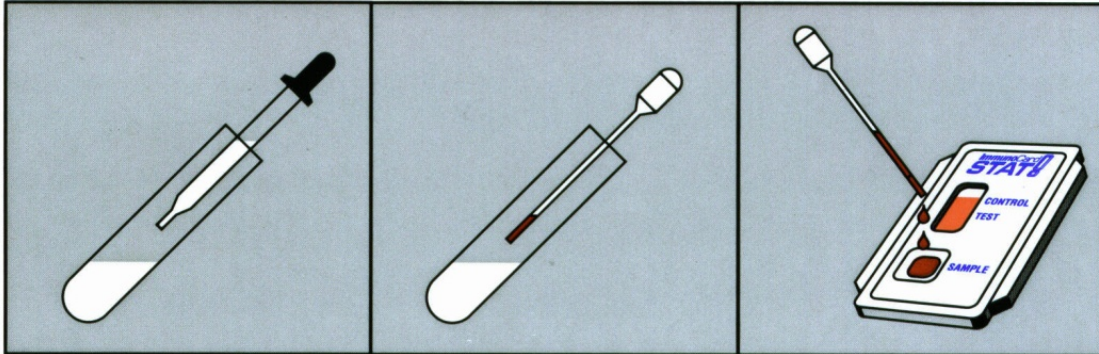


1. Add 350 µl of Sample Diluent to a test tube.

2 a. Add 25 µl of Stool Sample to the test tube. Mix well.
b. Add 350 µl of broth culture to the test tube. Mix well.

3. Add 150 µl of diluted sample to sample port. Incubate 10 minutes at 21°-25°C. Interpret Results.

INTERPRETATION OF RESULTS

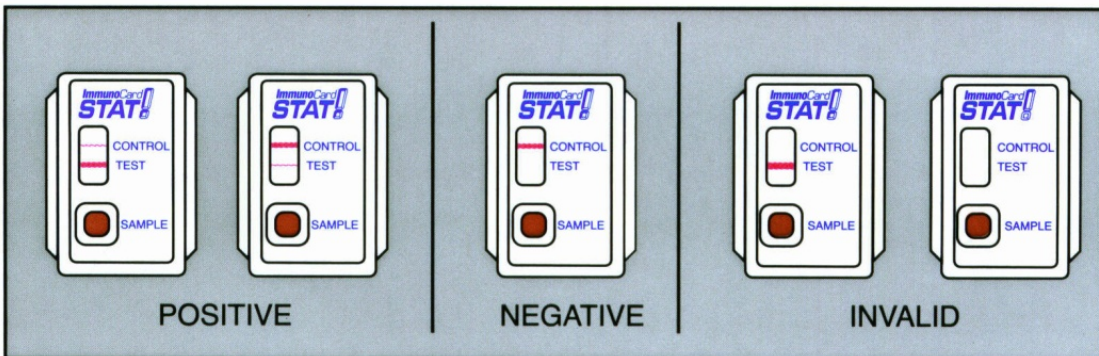

* This chart does not contain complete instructions for use. For further information, please refer to the package insert.